

Fig. 1

662020 "OFF THE SHELF"

66000" 0746360

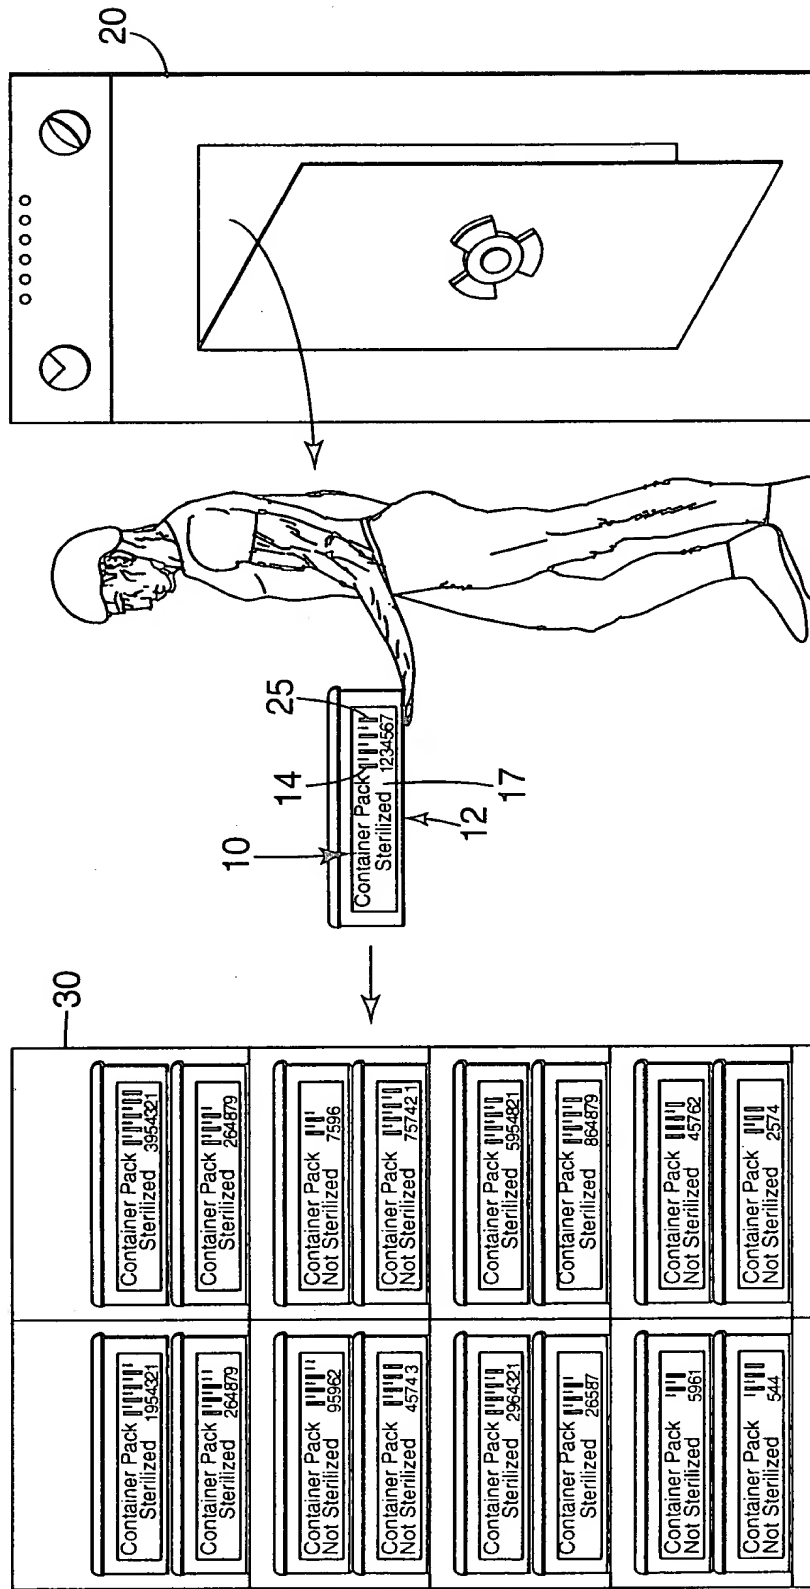


Fig. 2

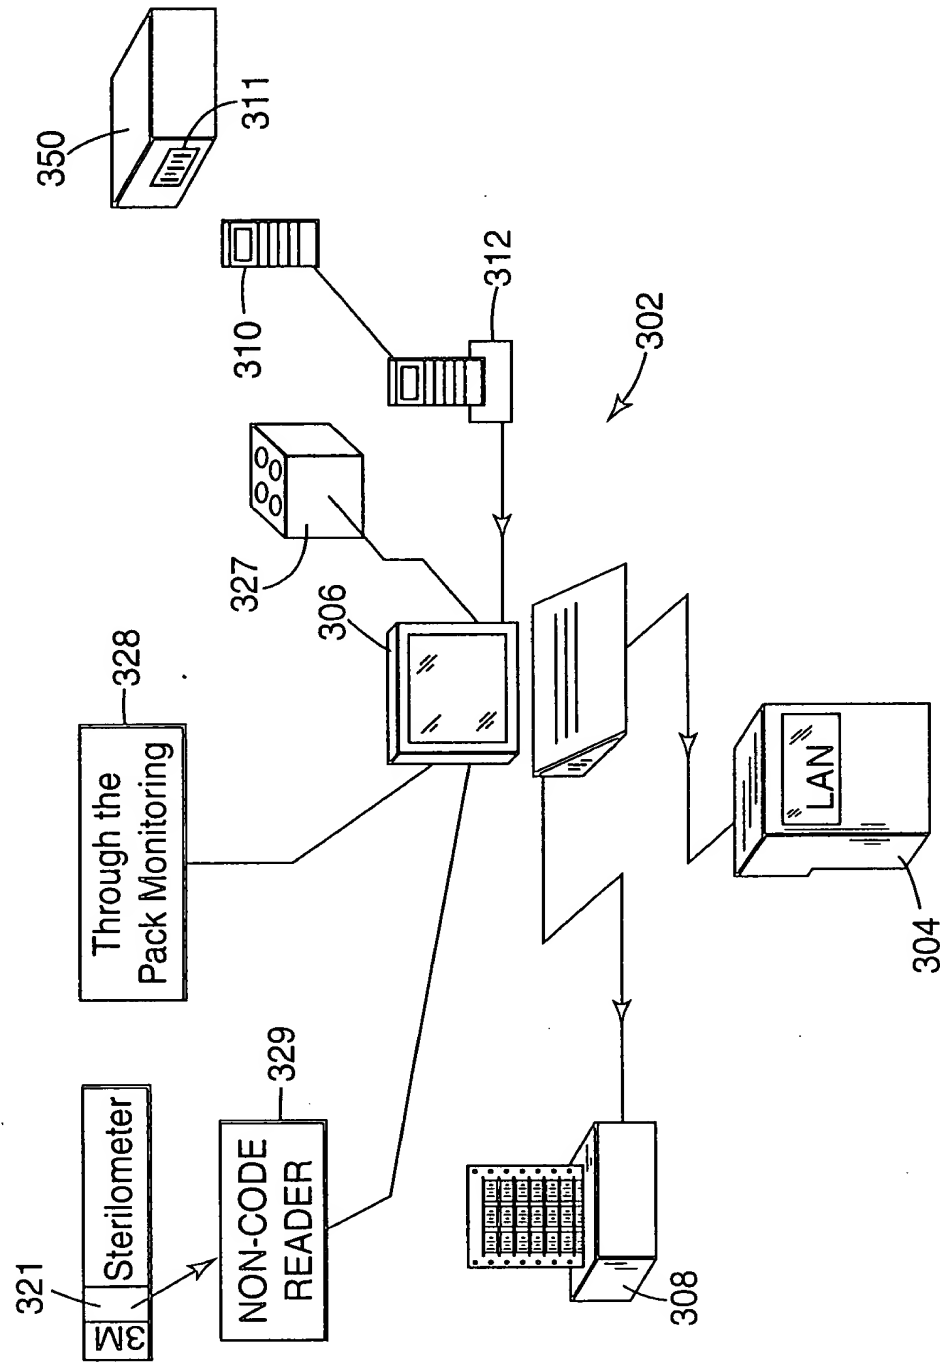


Fig. 4

662000" of 163200

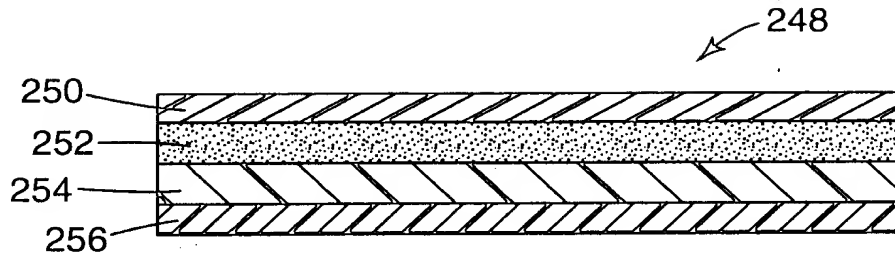


Fig. 5

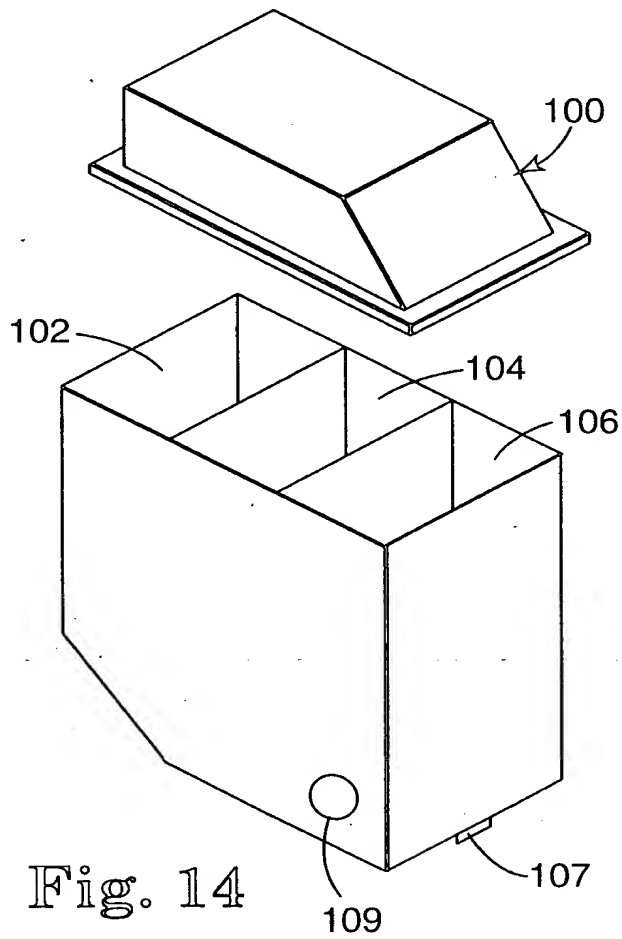


Fig. 14

66080 016360

| | | |
|-----------|-----------|----------|
| APPROVED | C.G. FIG. | |
| BY | CLASS | SUBCLASS |
| DRAFTSMAN | | |

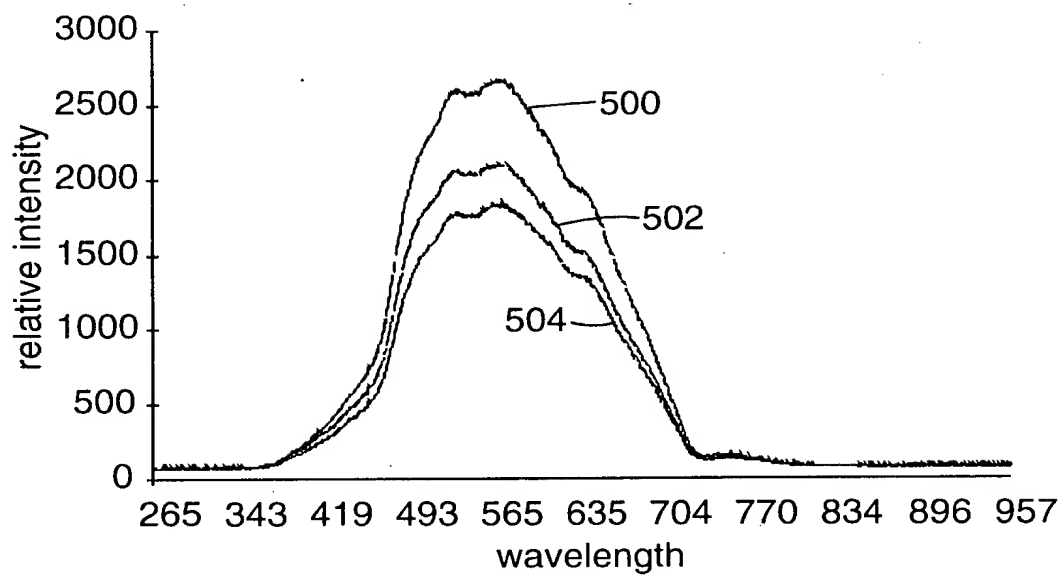


Fig. 6

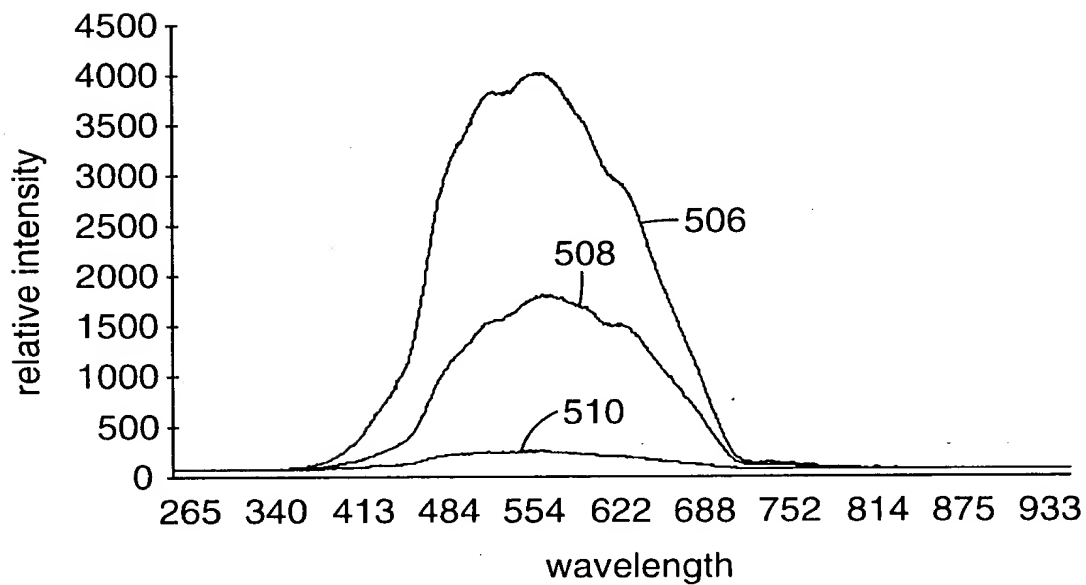


Fig. 7

662080-01109660

| | | |
|-----------|-----------|----------|
| APPROVED | C.G. FIG. | |
| BY | CLASS | SUBCLASS |
| DRAFTSMAN | | |

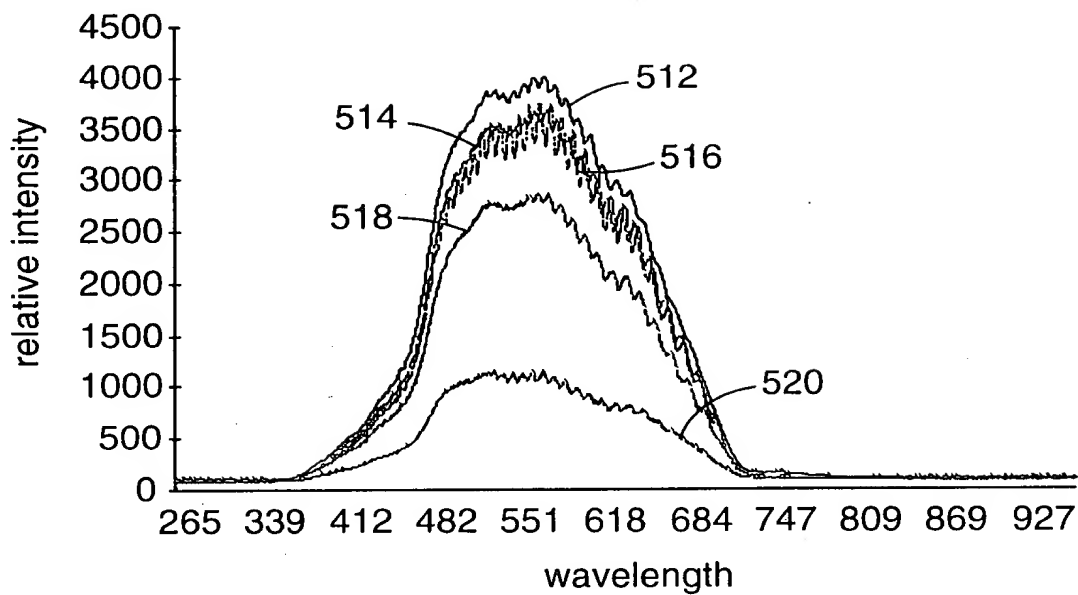


Fig. 8

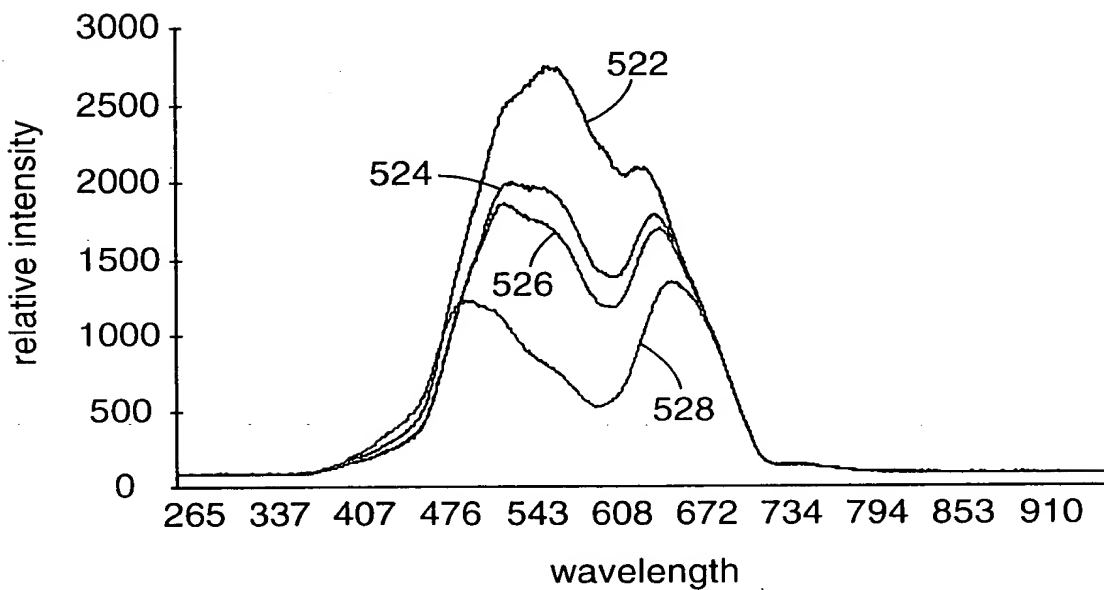


Fig. 9

66080" 07163260

| | | |
|-----------|-----------|----------|
| APPROVED | C.G. FIG. | |
| BY | CLASS | SUBCLASS |
| DRAFTSMAN | | |

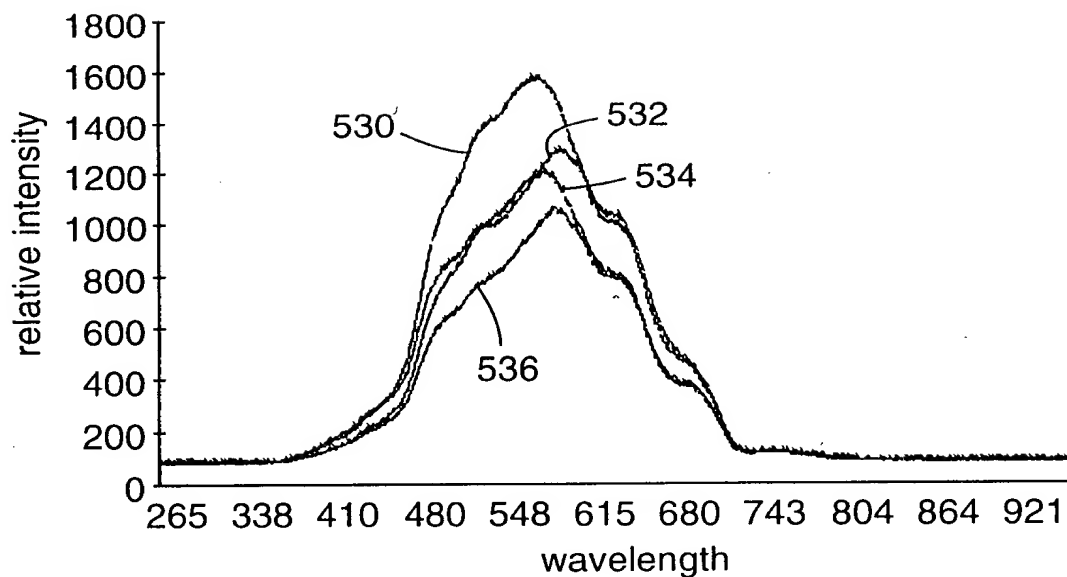


Fig. 10

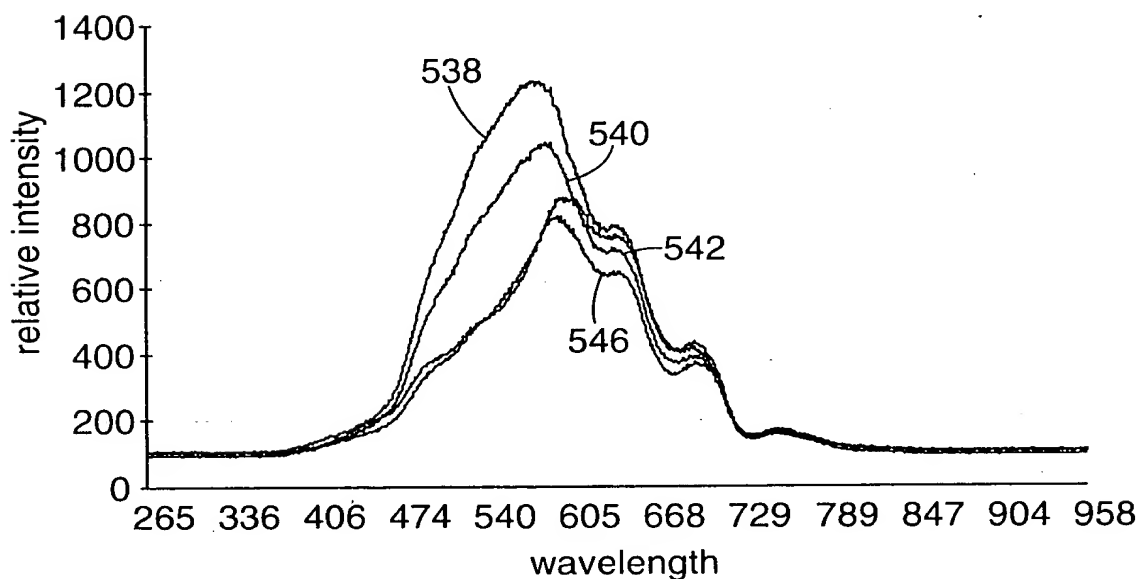


Fig. 11

662080 OF 16360

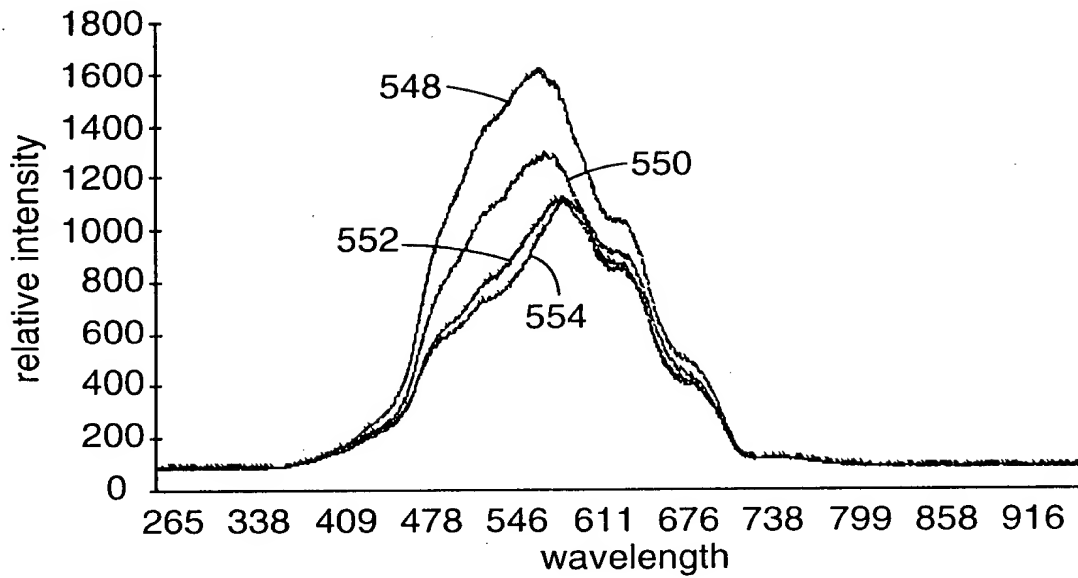


Fig. 12

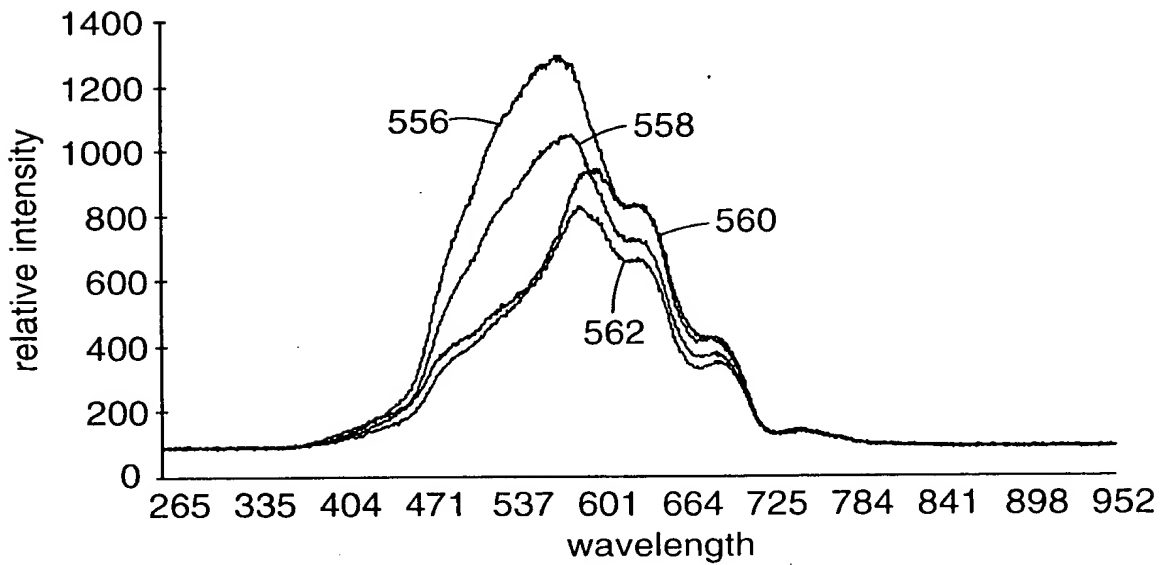


Fig. 13

66000 of 163600

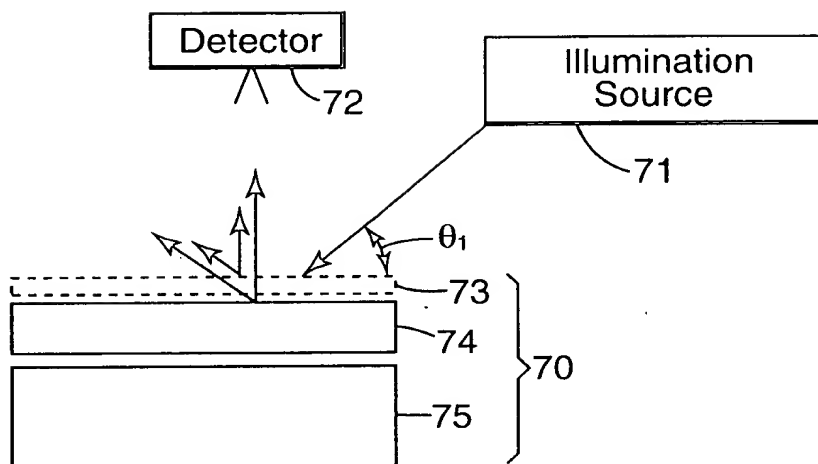


Fig. 15

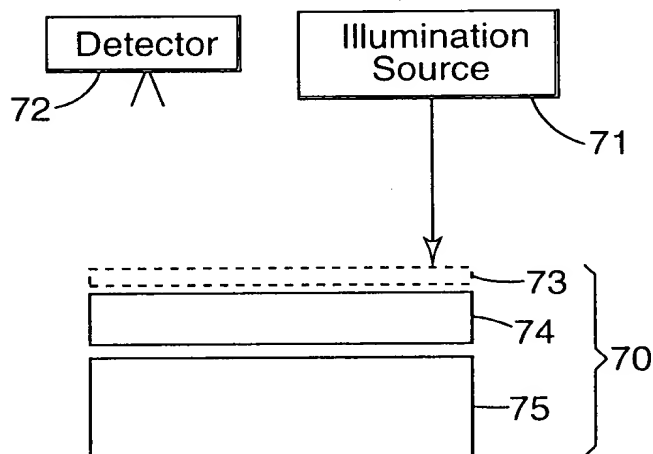


Fig. 16

662962 06163260

| | | |
|-----------|-----------|----------|
| APPROVED | C.G. FIG. | |
| BY | CLASS | SUBCLASS |
| DRAFTSMAN | | |

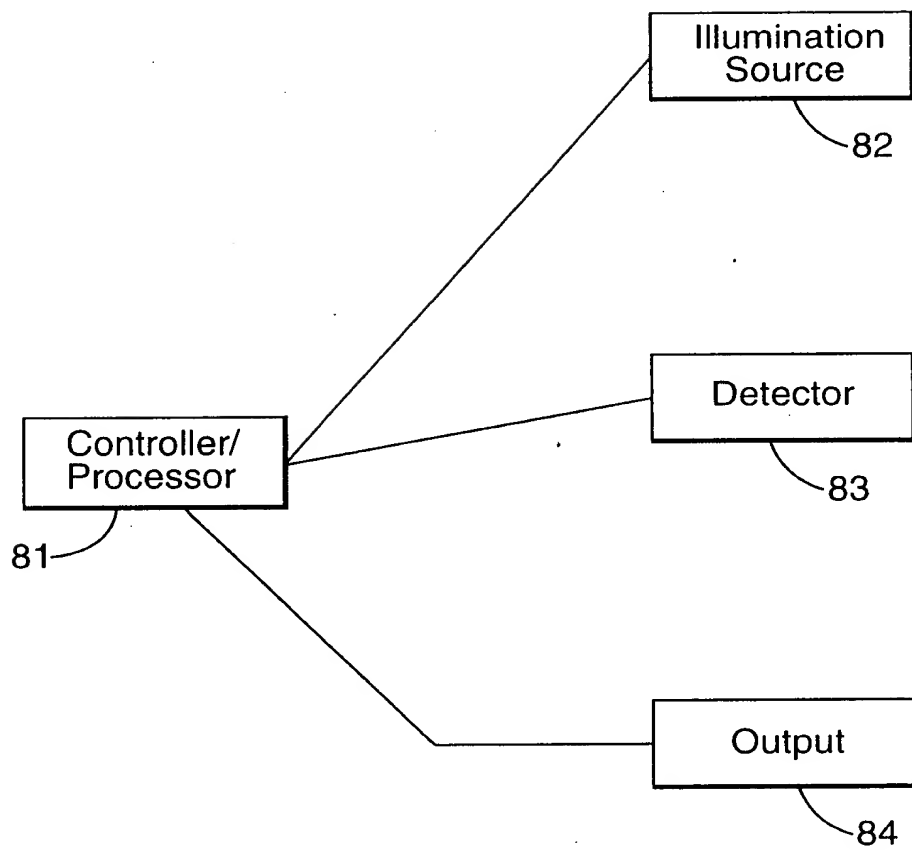


Fig. 17

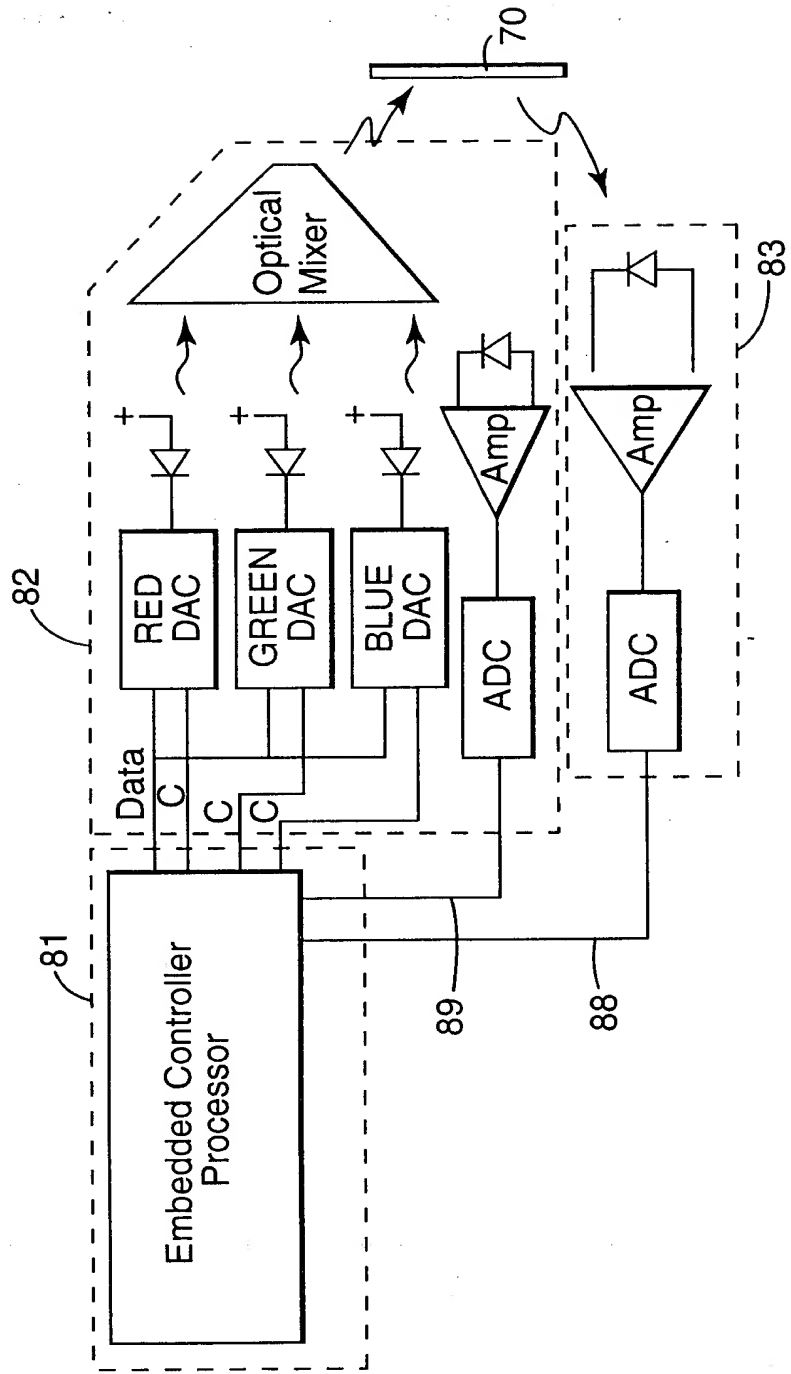


Fig. 18

| | | |
|-----------|-----------|----------|
| APPROVED | O.G. FIG. | |
| BY | CLASS | SUBCLASS |
| DRAFTSMAN | | |

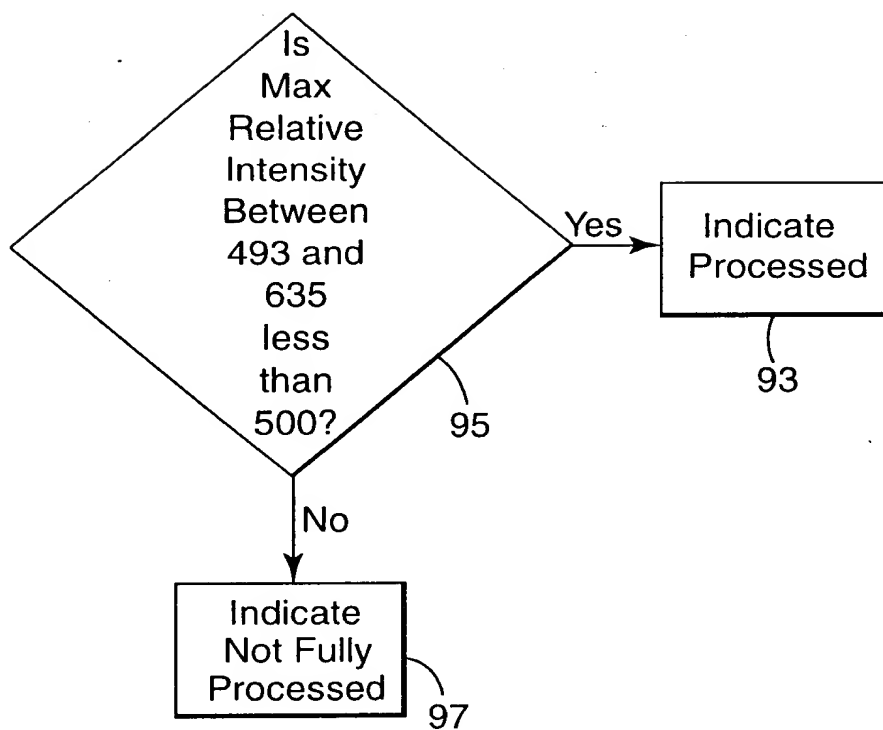


Fig. 19

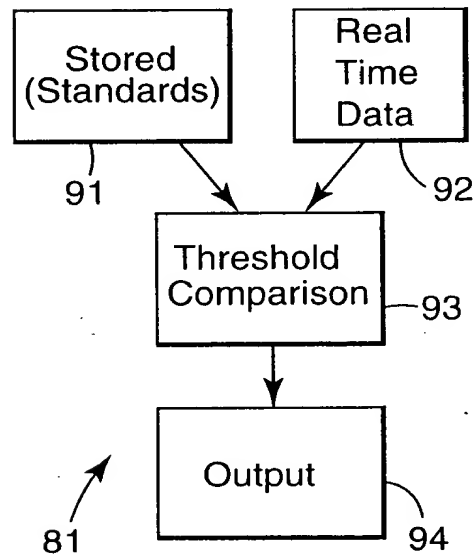


Fig. 20

66030" 07463600

| | | |
|-----------|-----------|----------|
| APPROVED | O.G. FIG. | |
| BY | CLASS | SUBCLASS |
| DRAFTSMAN | | |

☒ STATUS OF ARTICLES TO BE STERILIZED
☐ STERILIZATION INDICATORS
☐ CREATE A STERILIZATION PACK
☐ STERILIZERS

SELECT OPERATION AND THEN SELECT OK

OK

CANCEL

QUIT

Fig. 21

| | | |
|-----------|-----------|----------|
| APPROVED | C.G. FIG. | |
| BY | CLASS | SUBCLASS |
| DRAFTSMAN | | |

666000" 01163660

STERILIZER TYPE

☐ STEPPED Hydrogen Peroxide Plasma Sterilizer
 ☐ Steam Gravity Cycle
 ☒ Steam Vacuum Assist
 ☐ Flash Steam
 ☐ Steam-Vac (XL Sterilizer/Assistor (Ethylene Oxide))

SELECT TYPE OF STERILIZER AND SELECT CREATE TO MAKE A BAR CODE LABEL OF STERILIZATION INDICATOR INK

CREATE

CANCEL

QUIT

WHAT TYPE OF INDICATORS SHOULD I USE?

Fig. 22

| | | |
|-----------|-----------|----------|
| APPROVED | C.G. FIG. | |
| BY | CLASS | SUBCLASS |
| DRAFTSMAN | | |

☐ UNKNOWN LOCATION

☐ NEW PRODUCT
☐ CENTRAL STERILIZATION
☐ PROCESSED STORAGE
☐ DISTRIBUTION
☐ OPERATING ROOM
☐ DECONTAMINATION
☐ CLEAN ROOM ASSEMBLY
☐ DISCARD

OK

CANCEL

QUIT

SELECT LAST KNOWN
LOCATION

Fig. 23

| | | |
|-----------|-----------|----------|
| APPROVED | C. & FIG. | |
| BY | CLASS | SUBCLASS |
| DRAFTSMAN | | |

STERILIZATION
INDICATORS

STEAM VACUUM ASSIST

EXPOSURE CONTROL

PACKS SECURED WITH 3M COMPLY INDICATOR
TAPE NO.1222

LOAD CONTROL

3M RAPID ATTEST BIOLOGICAL INDICATORS NO. 1292

EQUIPMENT CONTROL

3M COMPLY BOWIE DICK PACK NO.1233

PACK CONTROL

3M COMPLY STERIGAGE STEAM CHEMICAL
INTEGRATOR NO. 1243 A OR B

Fig. 24

| | | |
|-----------|-----------|----------|
| APPROVED | C.G. FIG. | |
| BY | CLASS | SUBCLASS |
| DRAFTSMAN | | |

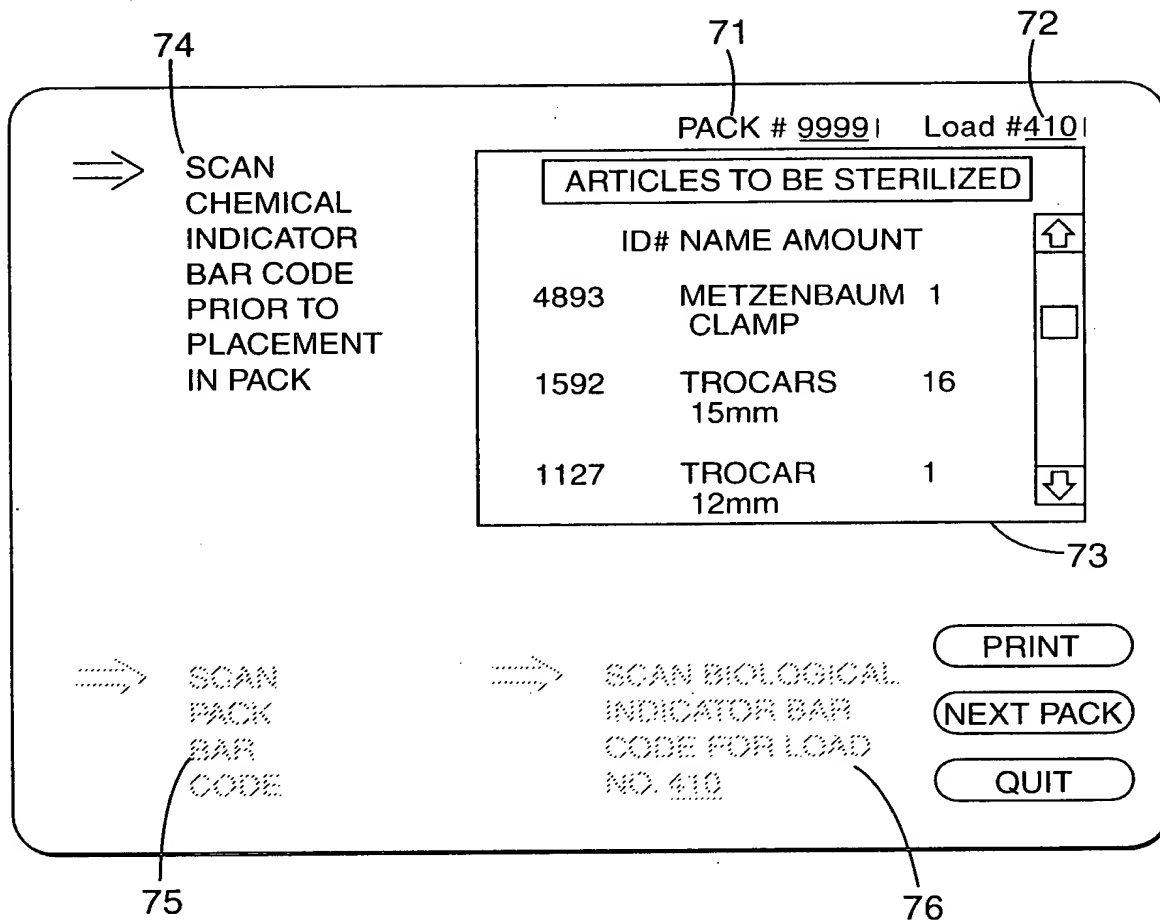


Fig. 25

| | | |
|-----------|-----------|----------|
| APPROVED | C.G. FIG. | |
| BY | CLASS | SUBCLASS |
| DRAFTSMAN | | |

WARNING!

PACK NO. 9999's CHEMICAL INDICATOR

READOUT IS INCONSISTENT WITH:

PACK NO. 8888's CHEMICAL
INDICATOR (SAME LOAD NO 410)

LOAD BIOLOGICAL INDICATOR NO.
410's BIOLOGICAL INDICATOR NO.

DO NOT USE CONTENTS BEFORE CONTACTING
CENTRAL STERILIZATION

Fig. 26

| | | |
|-----------|-----------|----------|
| APPROVED | C.G. FIG. | |
| BY | CLASS | SUBCLASS |
| DRAFTSMAN | | |

STEAM VACUUM ASSIST

391



CREATE A BAR CODE CHEMICAL
INDICATOR FOR PACK NO. 9999



SUGGEST STERILIZATION
INDICATOR SELECTION

ENTER

QUIT

Fig. 27

| | | |
|-----------|-----------|----------|
| APPROVED | C.R. FIG. | |
| BY | CLASS | SUBCLASS |
| DRAFTSMAN | | |

SURGICAL ARTICLES

STERILIZATION HISTORY

ID#

NAME

48931

METZENBAUM
CLAMP

LAST STERILIZED JUNE 3, 1999

SUBJECTED TO ☐ PREVIOUS
STERILIZATION CYCLES

LAST CYCLE READOUTS

BIOLOGICAL INDICATOR? OK

PACK CHEMICAL INDICATOR? OK

LOAD CHEMICAL INDICATOR? OK

Fig. 28

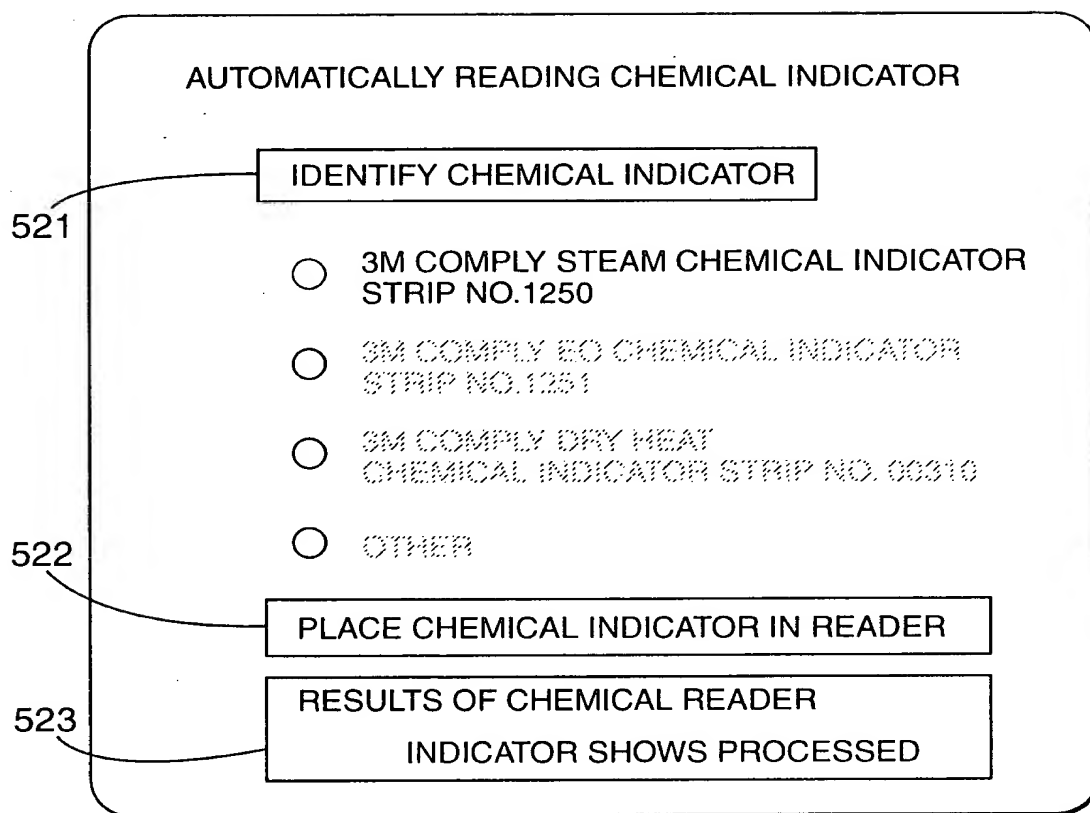


Fig. 29

| | | |
|-----------|-----------|----------|
| APPROVED | C.G. FIG. | |
| BY | CLASS | SUBCLASS |
| DRAFTSMAN | | |

410

| | |
|---------------------------------------|---------------------------------------|
| DEPARTMENT CODE _____ | HOSPITAL XYZ LABEL |
| PATIENT CHARGE CODE _____ | |
| IMPLANTABLE DEVICES _____ | |
| DATE AND TIME OF CYCLE _____ | BIOLOGICAL INDICATOR IN LOAD _____ |
| LOAD CONTENTS _____ | |
| EXPOSURE TIME AND CONCENTRATION _____ | |
| OPERATOR _____ | 6 7 8 9 1 |
| PACK NO. _____ | |
| LOAD NO. _____ | |
| Indicator Created By _____ | PURPLE=UNPROCESSED GREEN=PROCESSED |

CHEMICAL INDICATOR DESIGN

- ☐ BAR CODE — 405 ☐ OTHER — 407
- ☐ RECTANGULAR CONTINUOUS NON-CODE — 406

Backing

- ☐ Paper ☐ Other — 408
- ☐ Polymeric

STERILIZER

- ☐ HYDROGEN PEROXIDE — 401
- ☐ STEAM VACUUM ASSIST — 402
- ☐ STEAM GRAVITY — 403
- ☐ STEAM FLASH — 404

PROPER CARTRIDGE
LOADED IN PRINTER? OK

OTHER

- ☐ TYPE ADDITIONAL INFORMATION
- ☐ REMOVE INFORMATION

PRINT LABEL

Help Select Backing

MORE OPTIONS

QUIT

Fig. 30

| | | |
|-----------|-----------|----------|
| APPROVED | C.G. FIG. | |
| BY | CLASS | SUBCLASS |
| DRAFTSMAN | | |

66000" 07163600

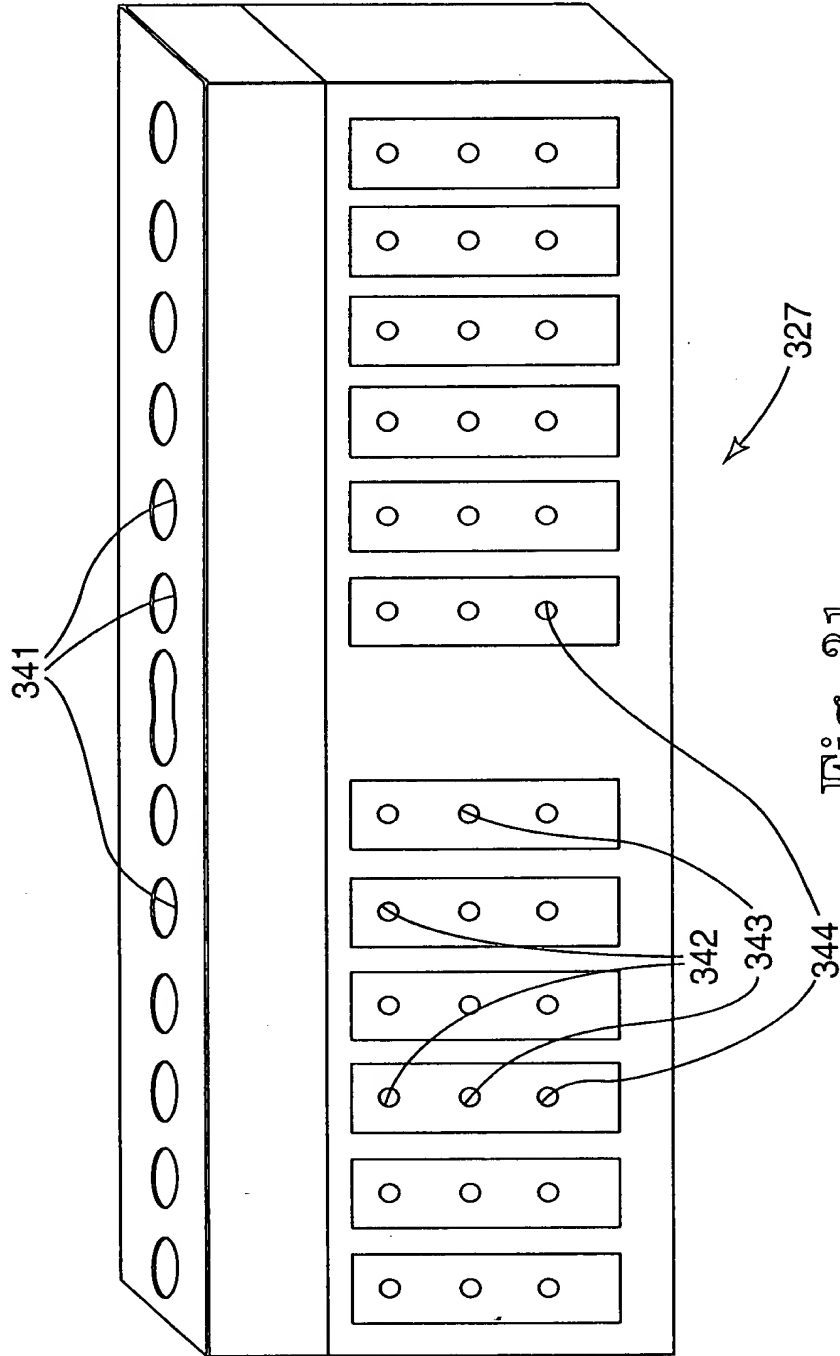


Fig. 31

